

Figure 1


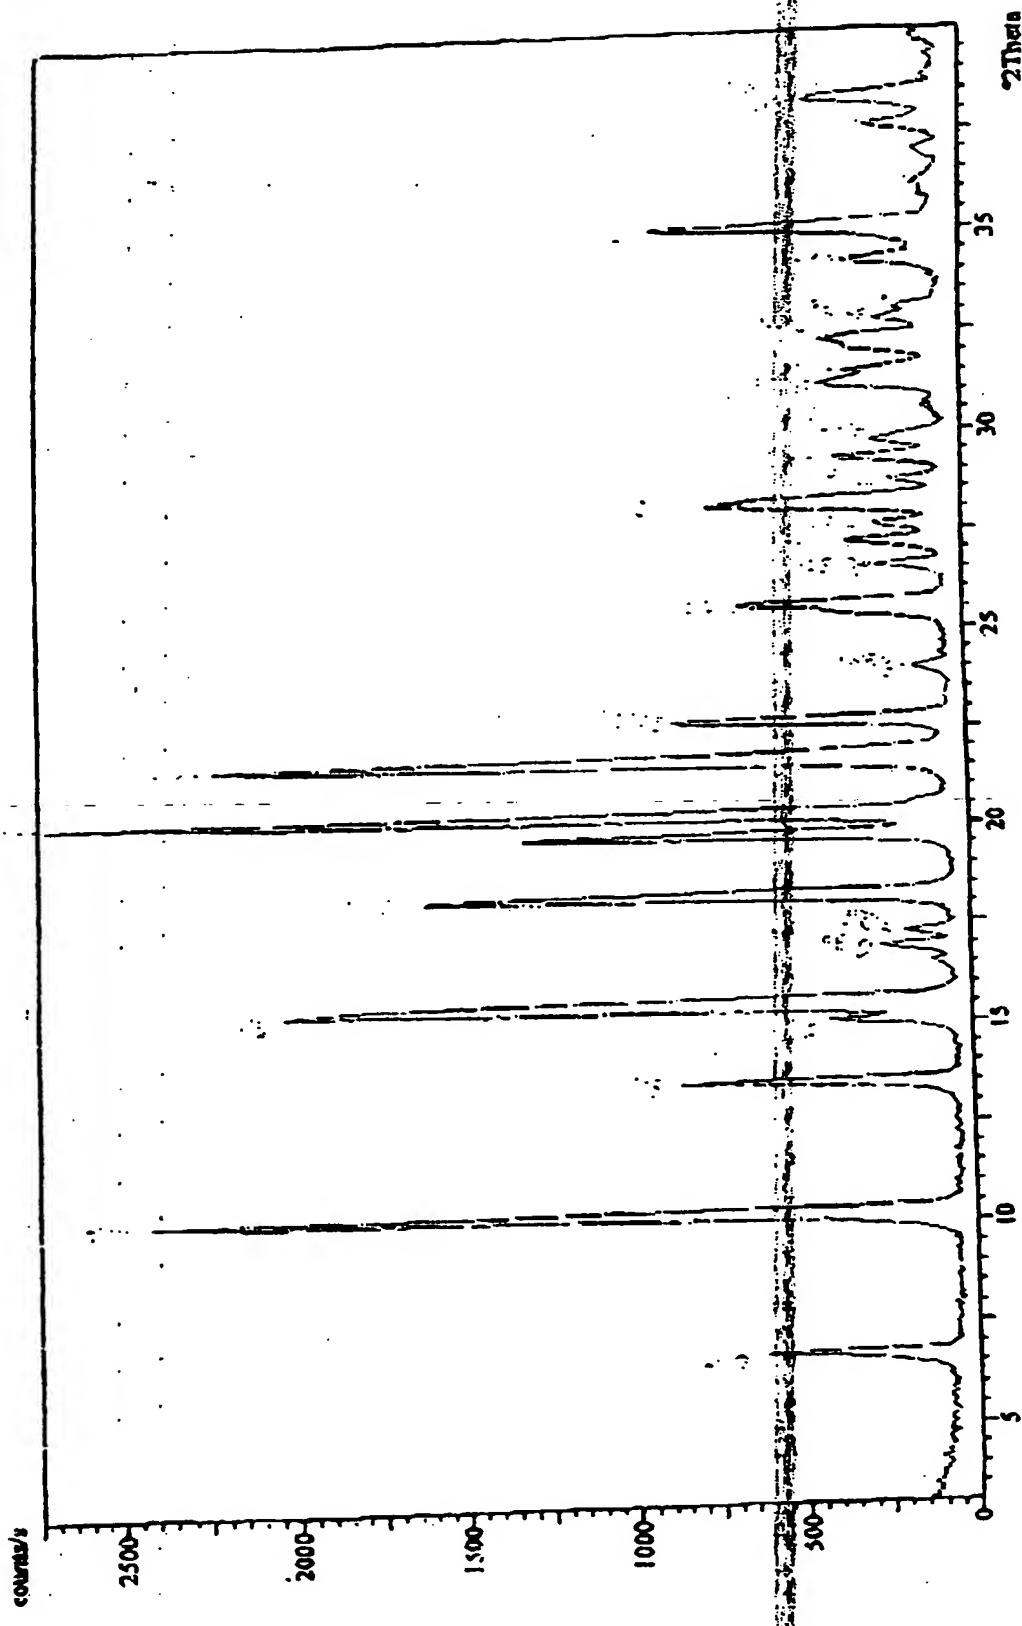


Figure 2

TO DATE 1992 450000 T

exo

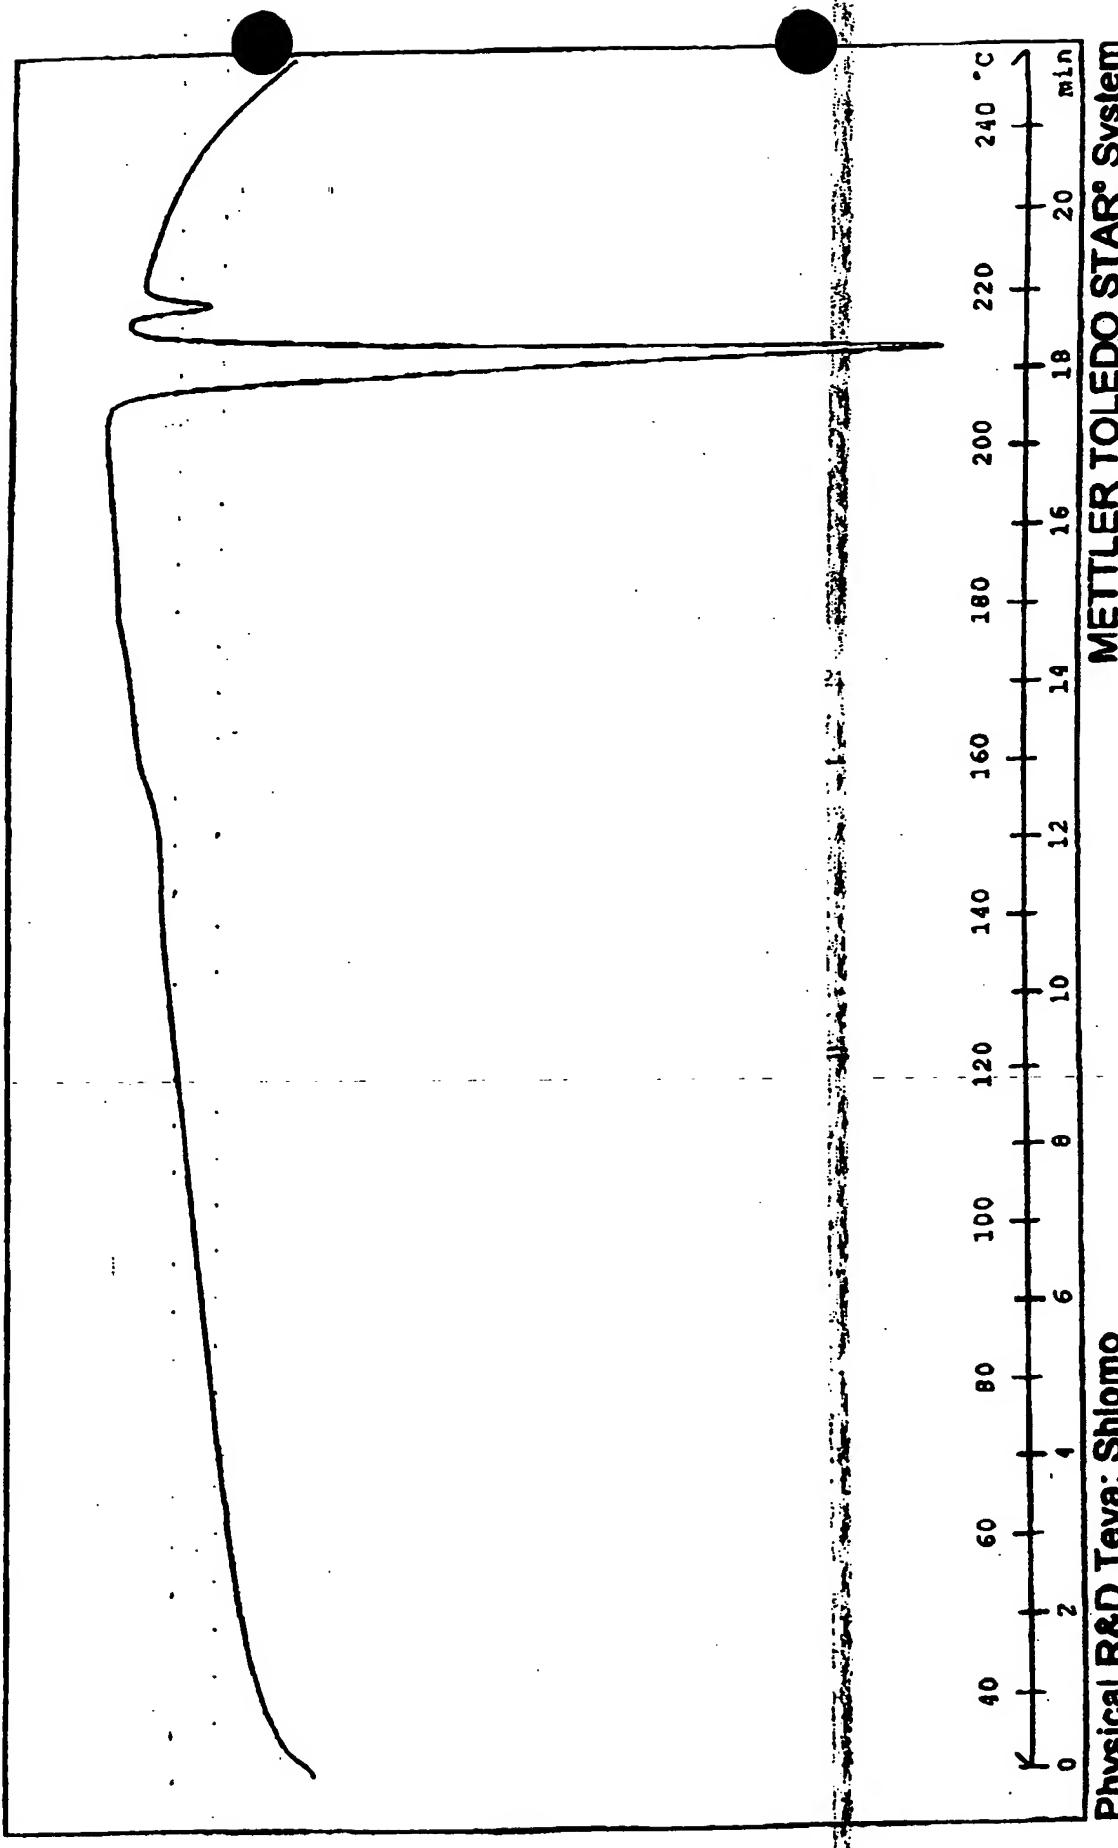

Physical R&D Teva: Shlomo

METTLER TOLEDO STAR® System

Figure 3

II


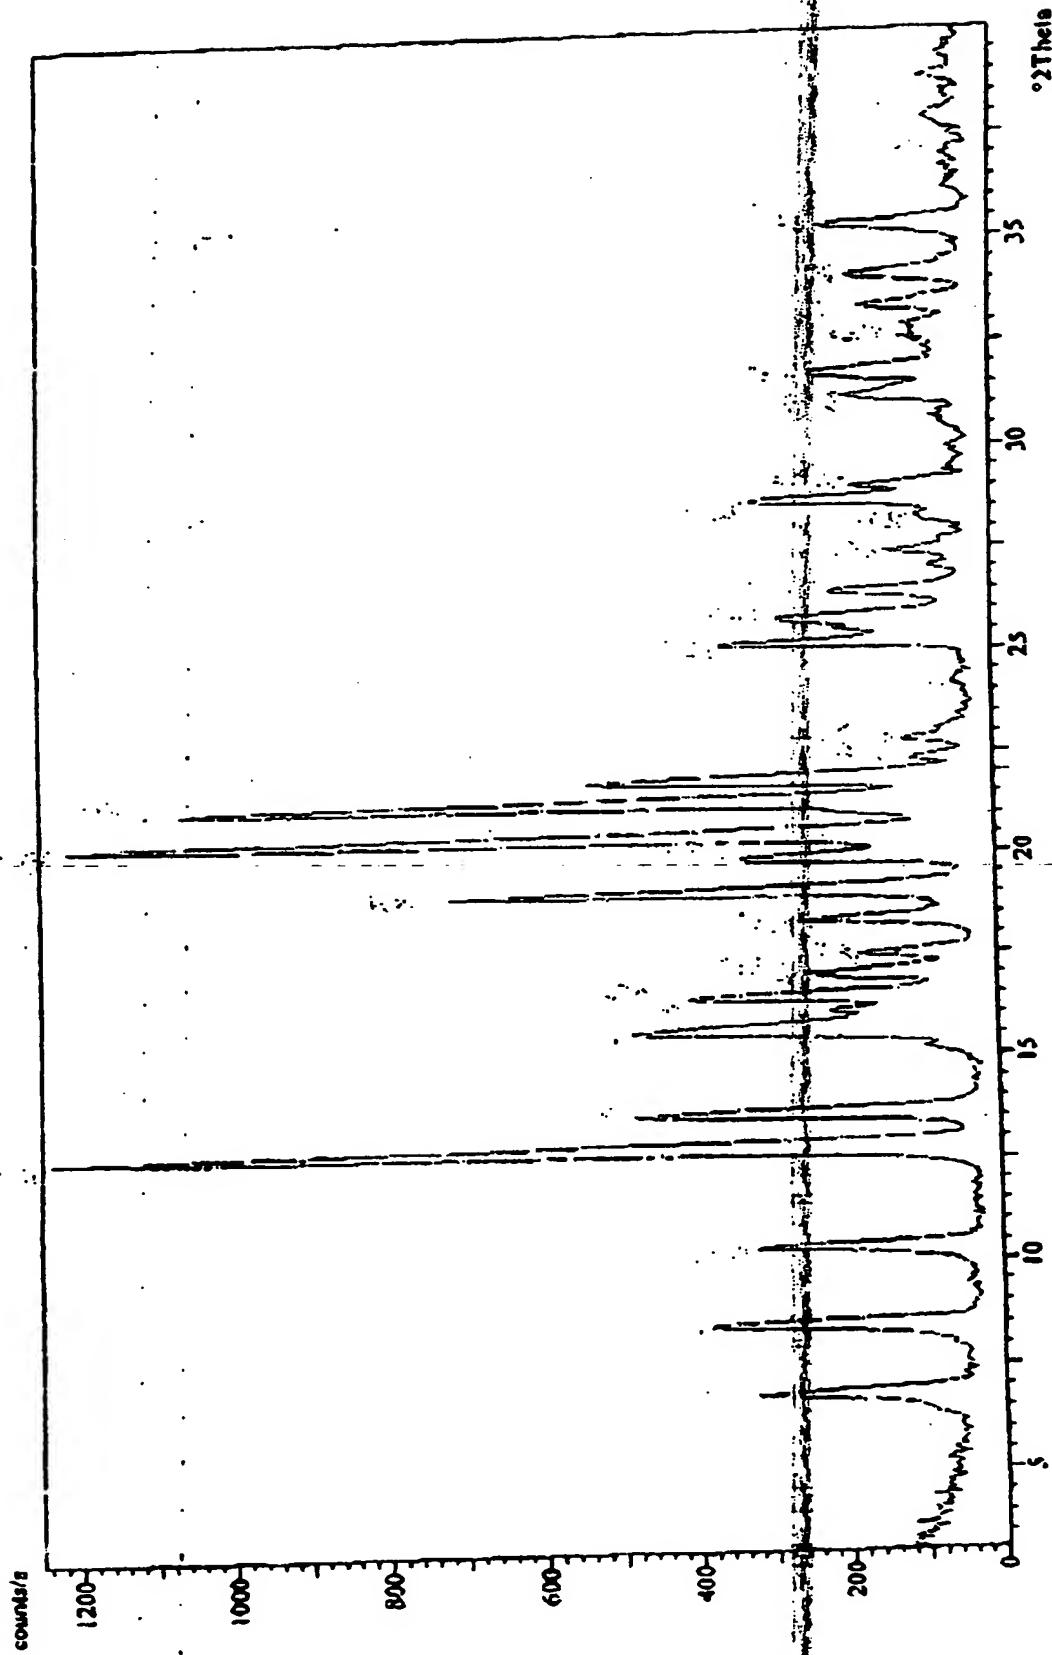


Figure 4

exo

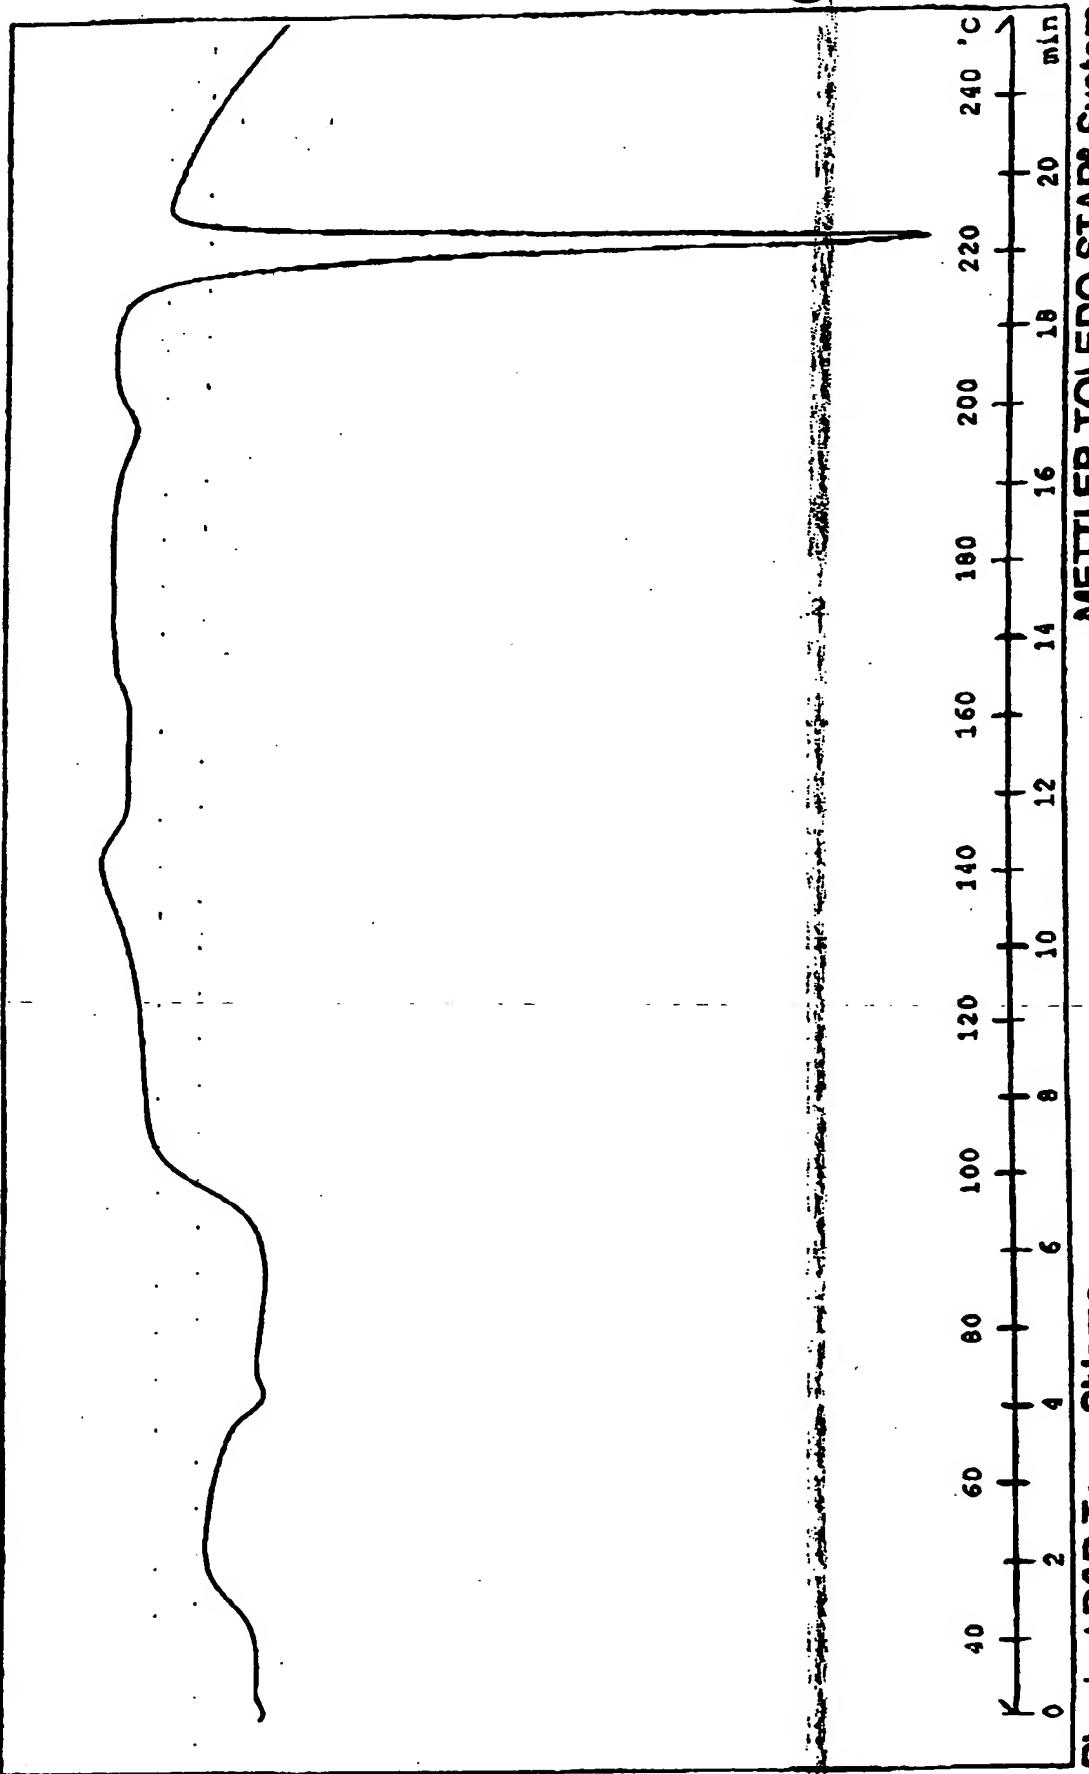

Physical R&D Teva: Shlomo

Figure 5

METTLER TOLEDO STAR® System

1000 800 600 400 200 0

TOTAL P.


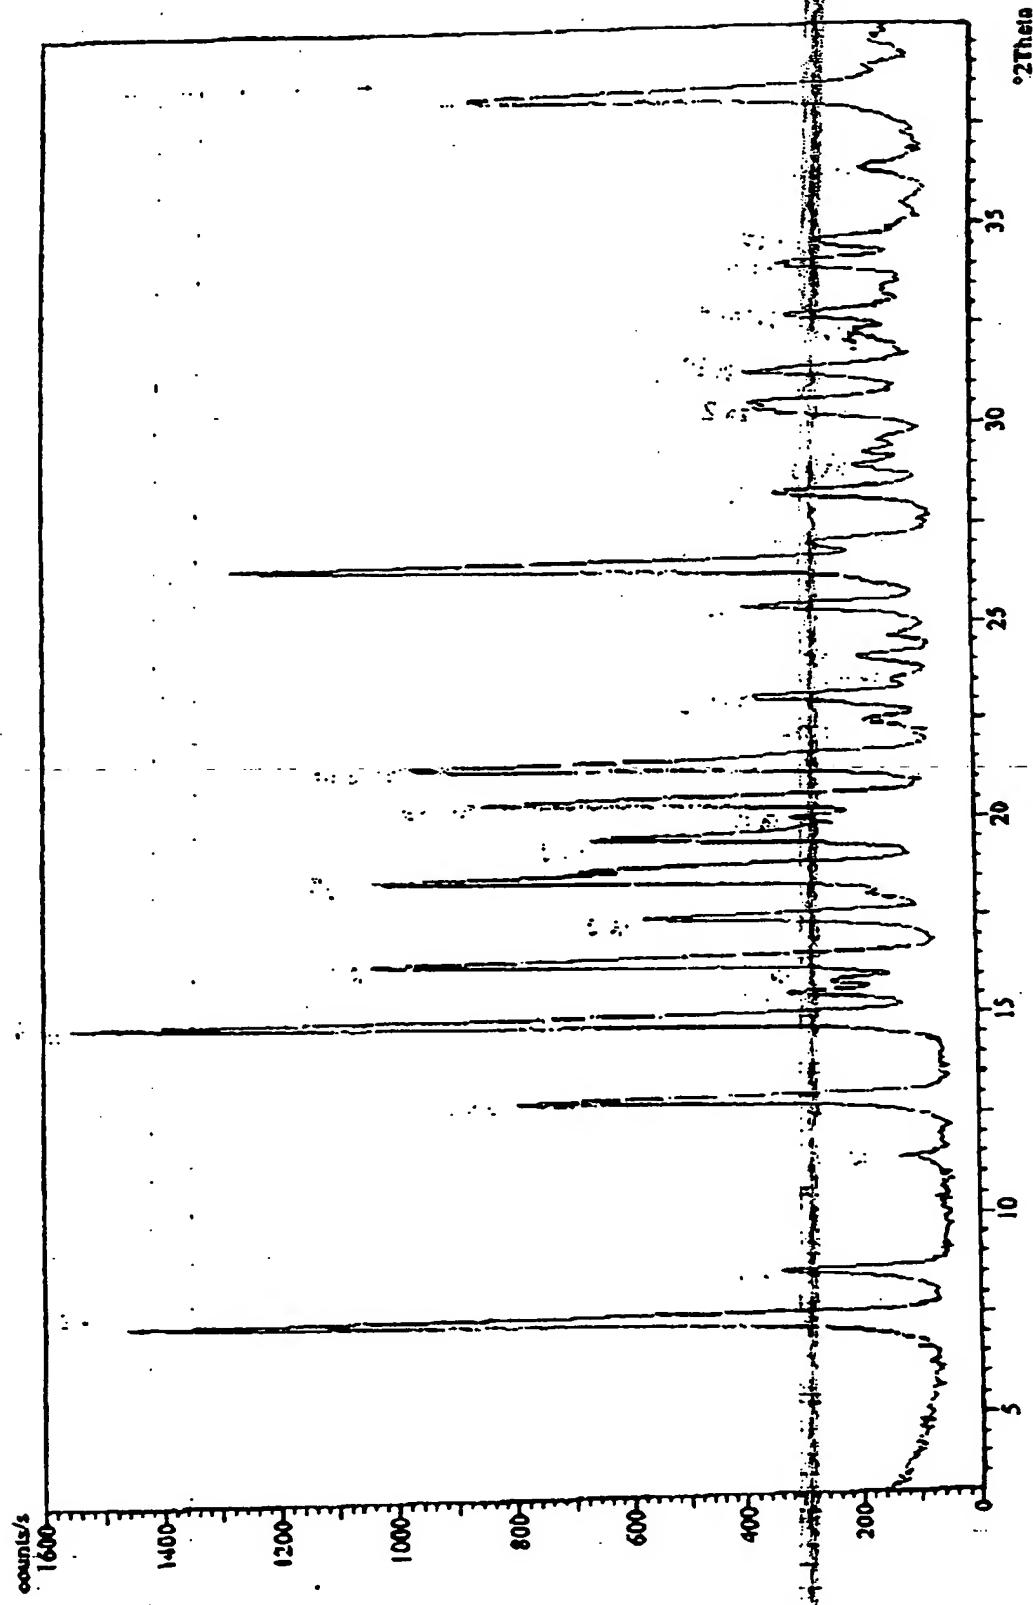


Figure 6

IV

ENDO

EXO

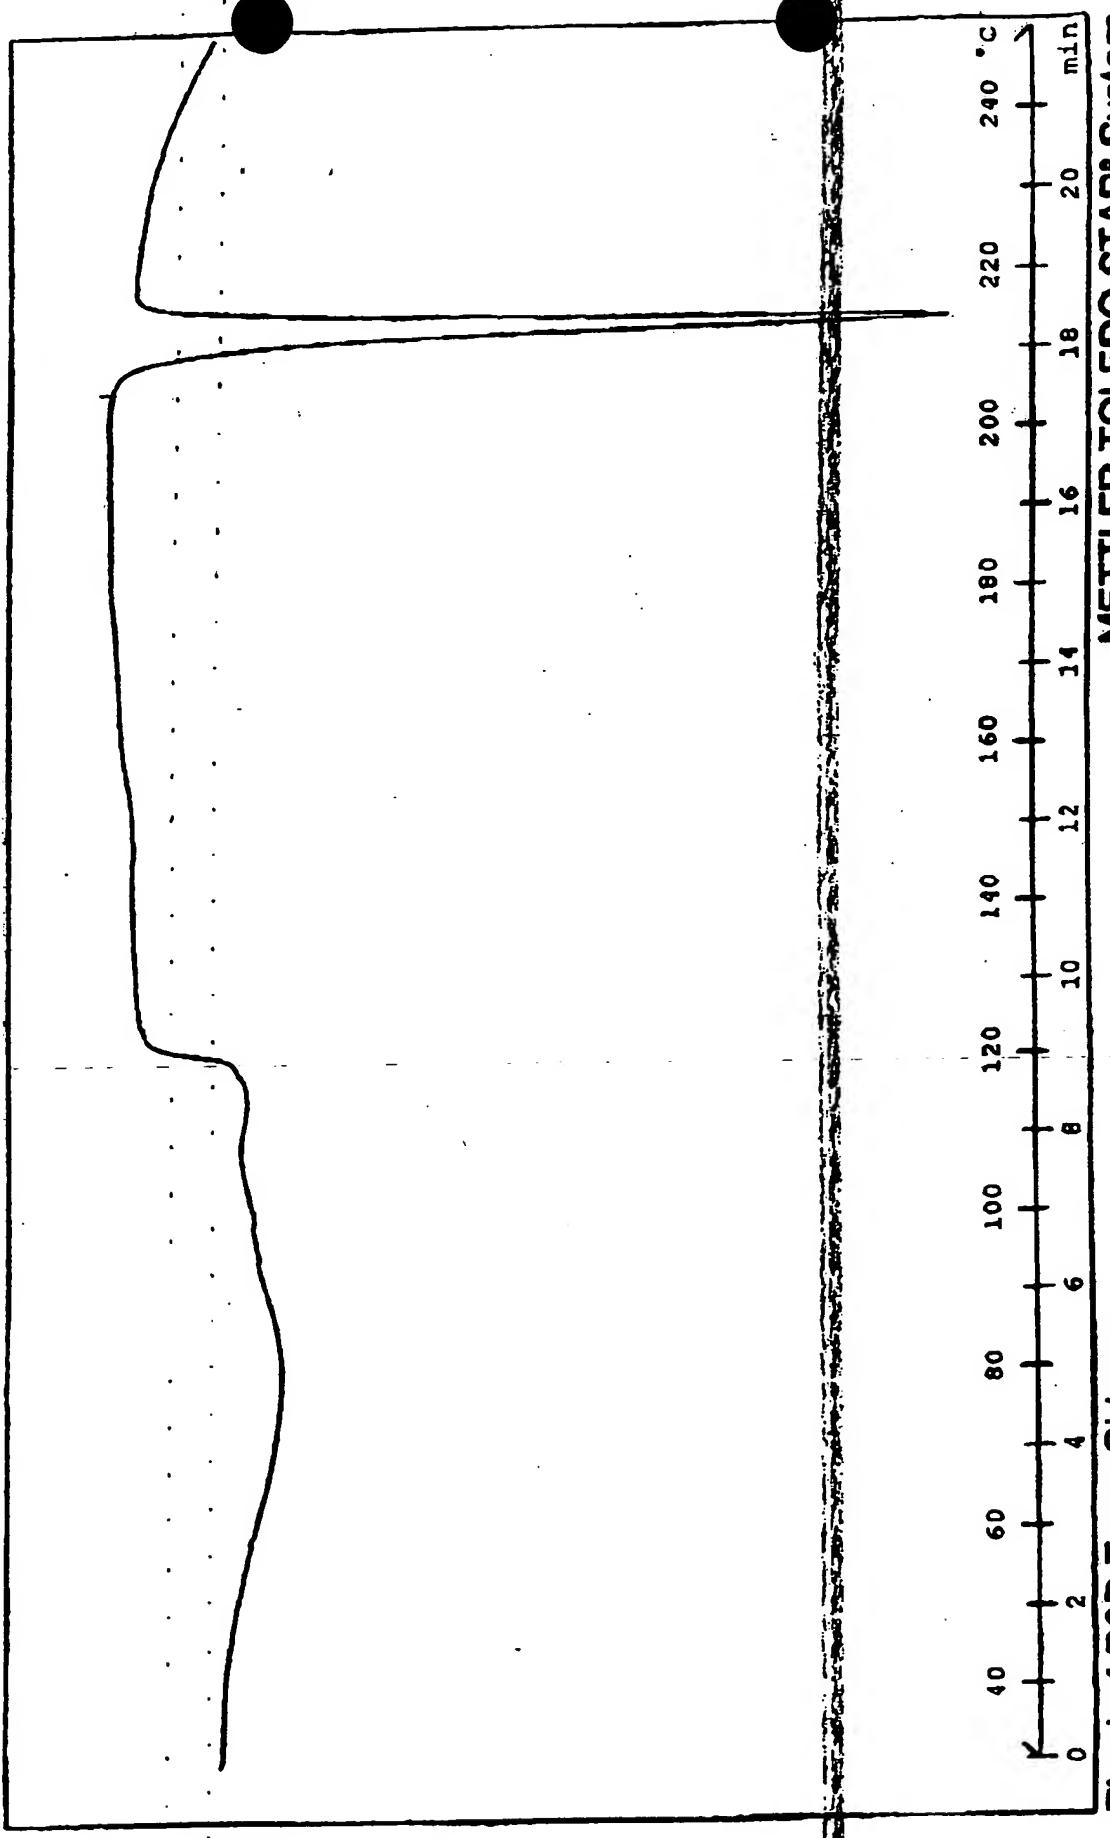

Physical R&D Teva: Shlomo

Figure 7

METTLER TOLEDO STAR® System

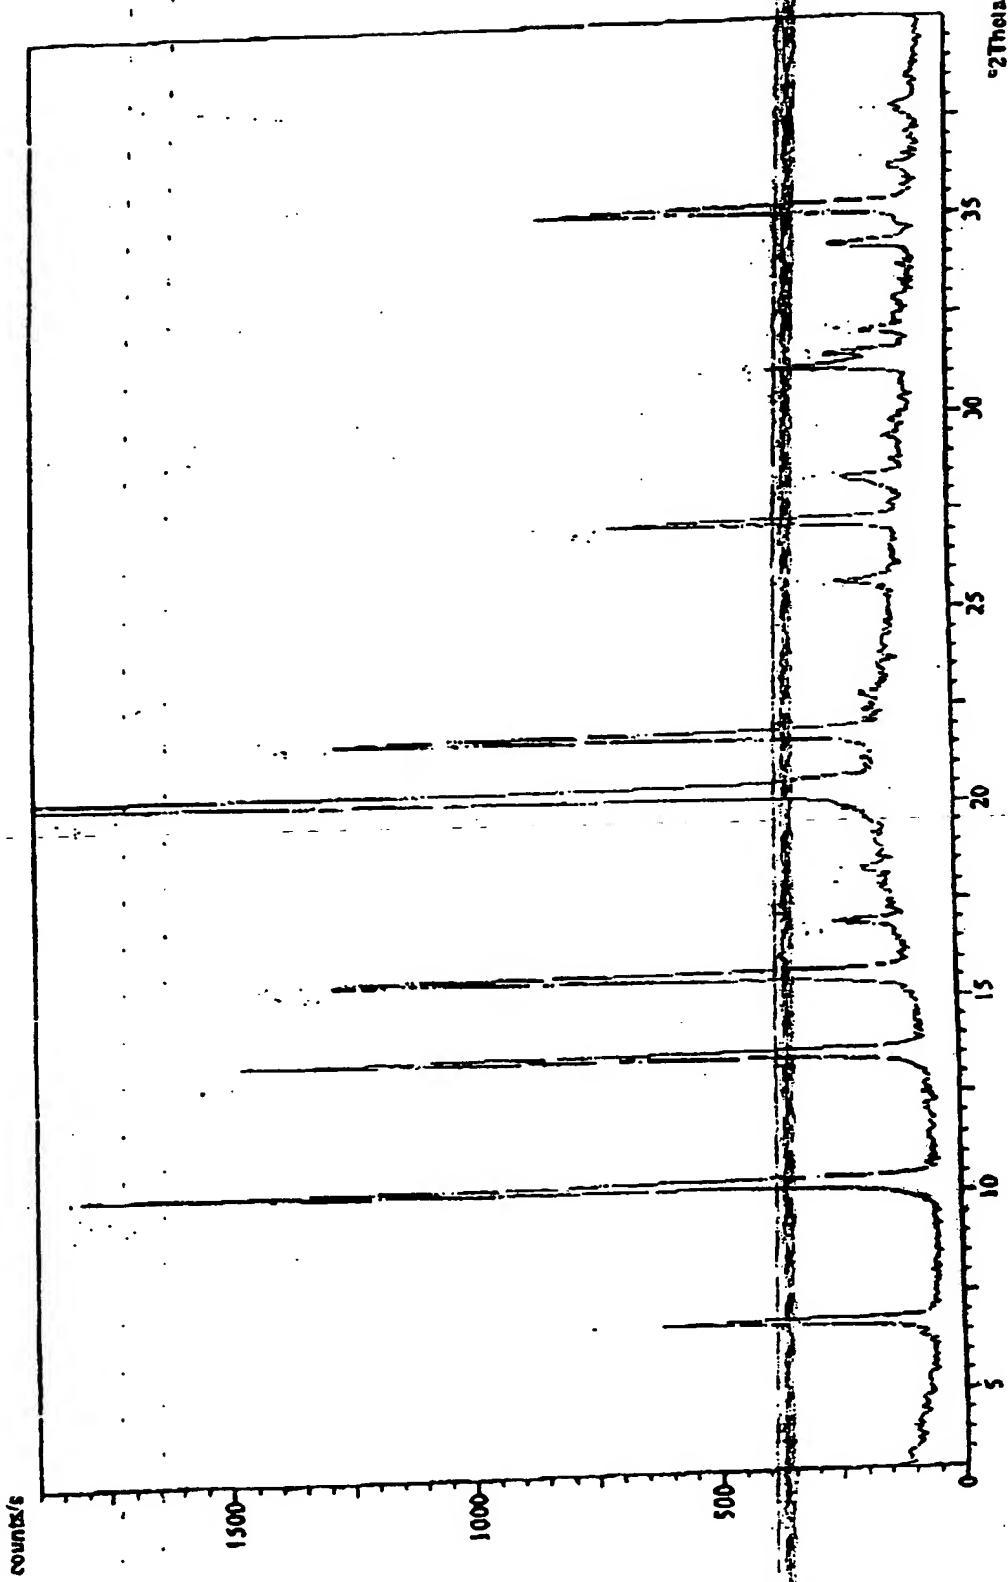


Figure 8

File: VEL-07 SHQ, ID: VEL-07 SHQ.
Date: 02/01/01 13:16 Step : 0.050° Cnt Time: 1.000 sec.
Range: 2.00 - 40.00 (Deg) Cont. Scan Rate : 3.00 Deg/min. TWA

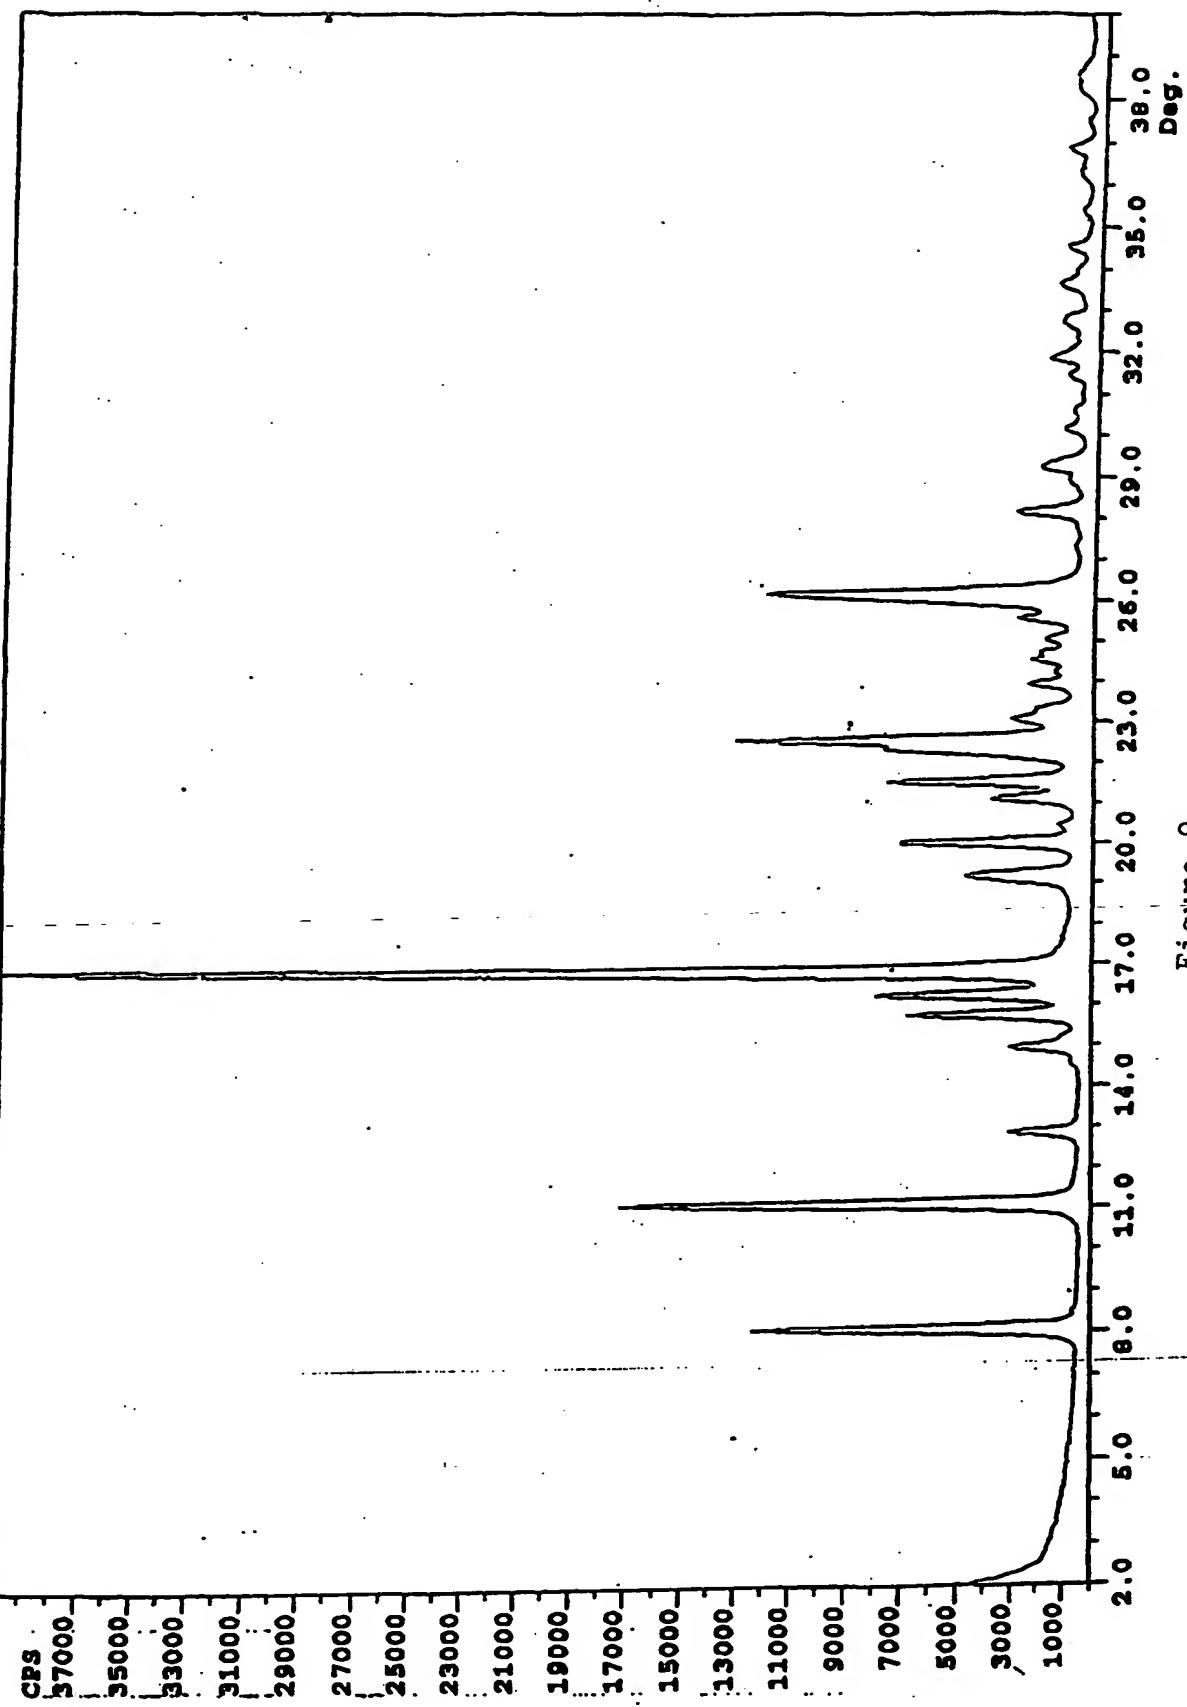


Figure 9

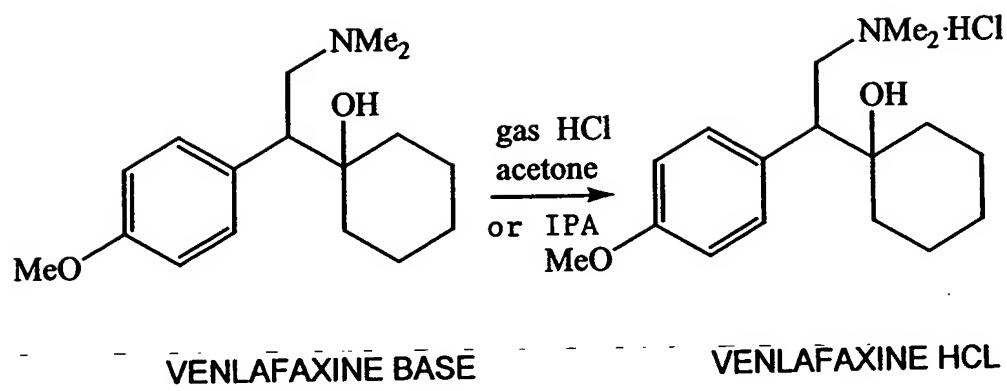


FIGURE 10